

SAM[®]

JUNCTIONAL TOURNIQUET

FOR BATTLEFIELD & TRAUMA INJURIES

NSN# 6515 01 618 7475

SAM
MEDICAL

SAM Medical Products[®]
27350 SW 95th Ave Ste 3038
Wilsonville, OR 97070 USA
503.639.5474 | sammedical.com


R_x only 2  CE
A single-use device

EC REP
Emergo Europe
Prinsessegracht 20, 2514 AP,
The Hague, The Netherlands

TO CONTROL DIFFICULT BLEEDS IN THE AXILLA AREA

Part No. SJT 102 Only

1. "click"

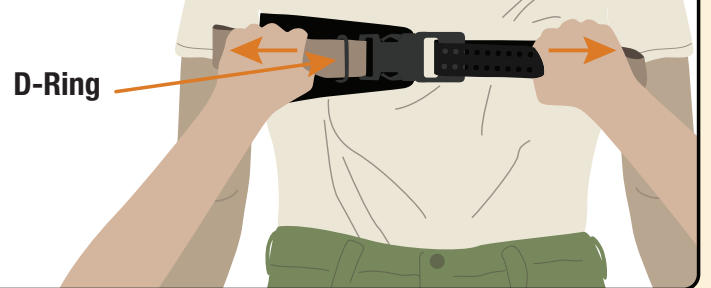


Apply the SJT to the patient under the arms, as high as possible. Place the D-ring on the injured side, aligning it with the side of the neck. Connect the buckle and secure the strap in place by pulling the **BROWN HANDLES** apart until you hear it click.

TO CONTROL DIFFICULT BLEEDS IN THE INGUINAL AREA


Part No. SJT 102,101

1.

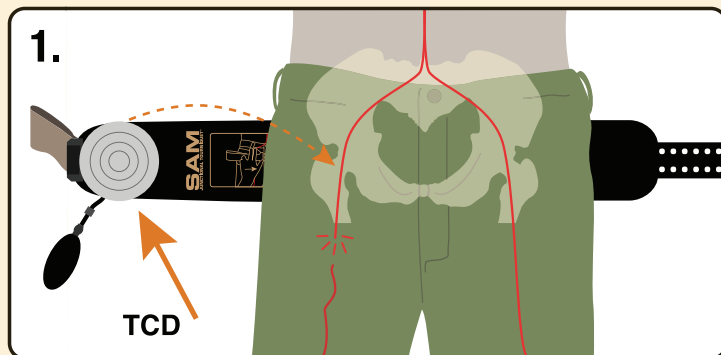


Slide the belt underneath the patient, positioning the Target Compression Device (TCD) over the area to be compressed. Use sterile gauze or hemostatic dressing if targeting directly over a wound. **For bi-lateral application, use a second TCD.**

2.

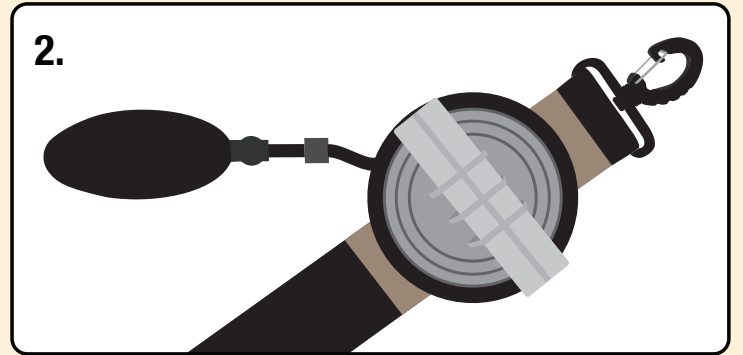


Attach the Extender to the TCD prior to application and place on the strap on the brown velcro.

2.

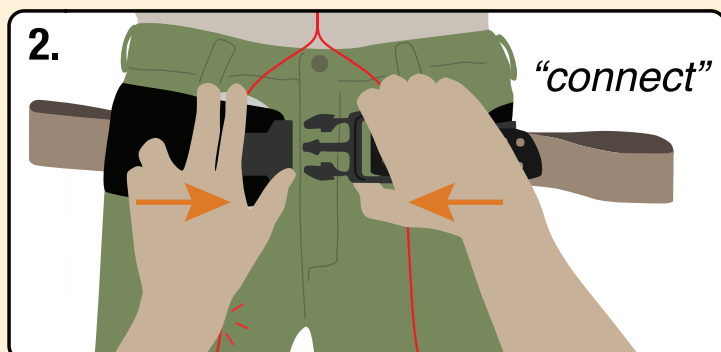


Hold the TCD in place and connect the belt using the buckle.

3. "connect"

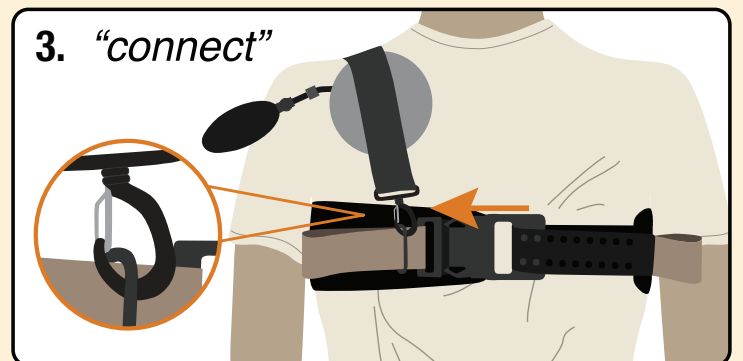

Connect the strap using the large clip to the D-ring on the front of the SJT.

3.

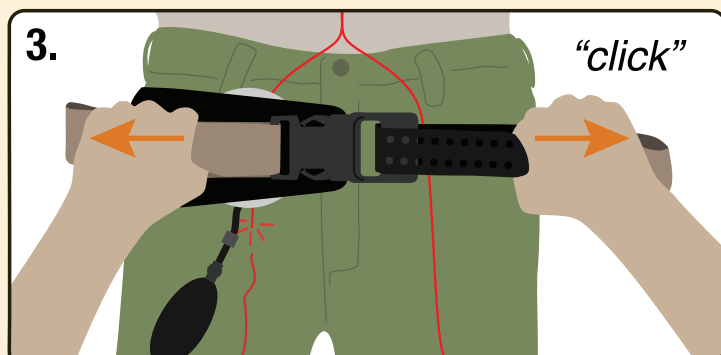


Pull the **BROWN HANDLES** away from each other until the buckle secures. You will hear an audible click. Fasten excess belt in place by pressing it down on the Velcro. You may hear a second click once the belt is secure.

4.




Connect the auxiliary strap to the cord on the back of the SJT using the small clip, as close as possible to the patient's mid-line.

4.

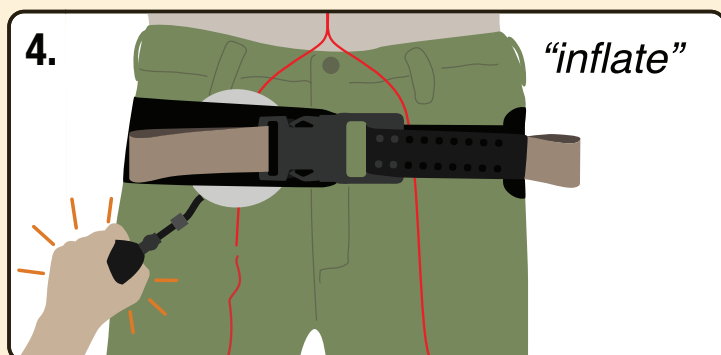

Use the hand pump to inflate the TCD until hemorrhage stops. Monitor patient during transport for hemorrhage control and adjust the device if necessary. **TO REMOVE**, unbuckle the belt.

5.

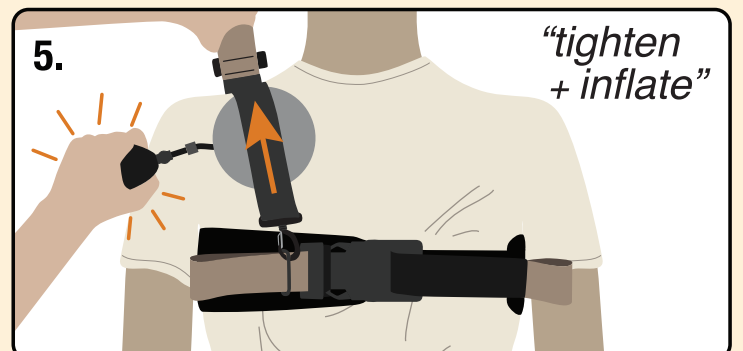

Tighten the strap as much as possible using the **BROWN HANDLE**.

Use the hand pump to inflate the TCD until hemorrhage stops. Monitor patient during transport for hemorrhage control and adjust the device if necessary. **TO REMOVE**, unbuckle the belt.

SAM[®]

JUNCTIONAL TOURNIQUET

FOR BATTLEFIELD & TRAUMA INJURIES

NSN# 6515 01 618 7475

SAM[®]
MEDICAL


SAM Medical Products[®]
27350 SW 95th Ave Ste 3038
Wilsonville, OR 97070 USA
503.639.5474 | sammedical.com

R_x only **2**  **CE**
A single-use device


EC REP
Emergo Europe
Prinsessegracht 20, 2514 AP,
The Hague, The Netherlands

TO IMMOBILIZE A PELVIC FRACTURE


Part No. SJT 102, 101, 100

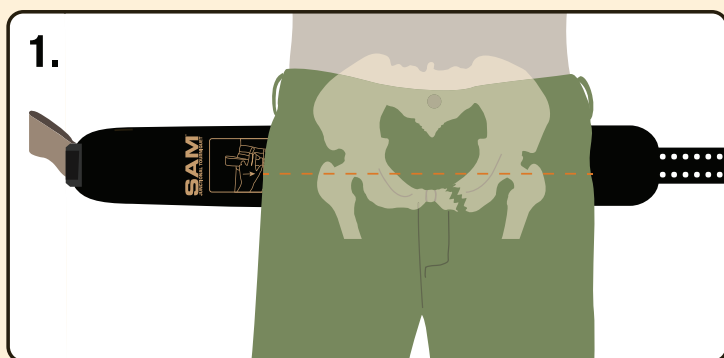

Remove objects from patient's pockets or pelvic area. Slide the belt without the TCD underneath the patient at level of the trochanters (hips).

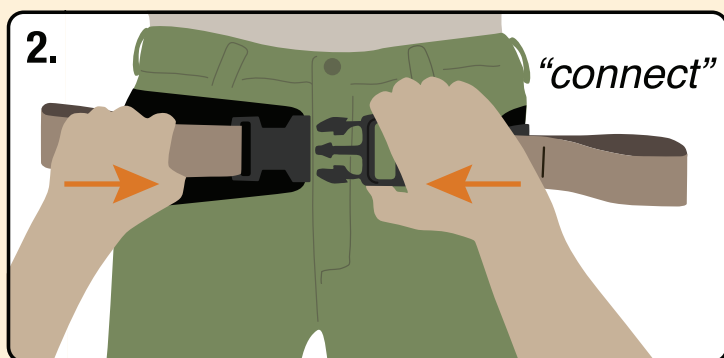

Connect the belt using the buckle.

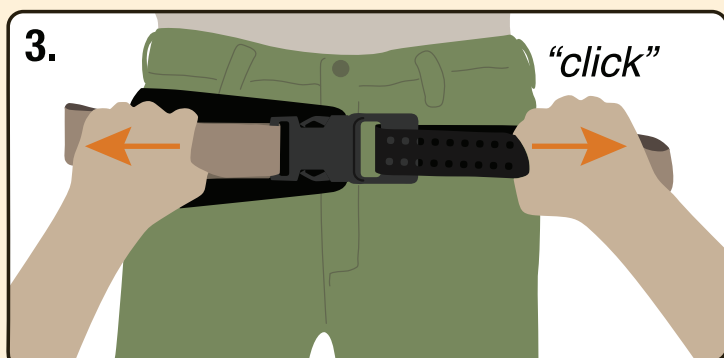

Pull the **BROWN HANDLES** away from each other until the buckle secures. You will hear an audible click. Fasten excess belt in place by pressing it down on the Velcro. You may hear a second click once the belt is secure. In case of prolonged use, monitor patient's skin.

When used as a pelvic sling, the SJT should remain firmly attached to the patient while in the MRI room.

TO REMOVE, unbuckle the belt.

Part No.	Description
SJT 102	SJT, 2 TCD, Ext, Hand Pump, Aux Strap
SJT 101	SJT, 1 TCD & Hand Pump
SJT 100	Pelvic Sling

WARNING: The SAM[®] Junctional Tourniquet is intended to be left on for up to four hours. Remove only at a Definitive Care Facility. Additional hand pumps may be necessary with changes in altitude.

Note: If altitude change is a concern, a syringe can be used to fill the TCD with water, saline, or other non-compressible fluid.

Rev # SJT-203-05



6 80569 71735 1